

# TEST REPORT

(Electronic version)



No:200081167

VERIFICATION WEBSITE: [www.gttc.net.cn](http://www.gttc.net.cn)

VERIFICATION CODE: KFHE-4321-24

ISSUE DATE:2020-04-15

扫码下载报告



APPLICANT: AAB(CHINA)CO.,LTD  
ADDRESS: AAB Industrial Park, Honglai Town, Nan'an City, Fujian Province, China.

## INFORMATION CONFIRMED BY APPLICANT:

KN95 PROTECTIVE

QUANTITY: FIFTY PIECES

BRAND: AAB

COLOUR: WHITE

MANUFACTURE'S NAME: AAB(CHINA)CO.,LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-15

## CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
APPEARANCE INSPECTION[2 PIECES]	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT  
"---" -NO COMMENT

## REMARK:

THE AUTHORIZATION OF APPEARANCE INSPECTION IS NOT RECEIVED FROM CNAS.  
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200062093.  
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).  
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.  
THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山



PAGE 1 OF 4

# TEST REPORT

(Electronic version)


No:200081167



TEST REPORT

(Electronic version)

No:200081167

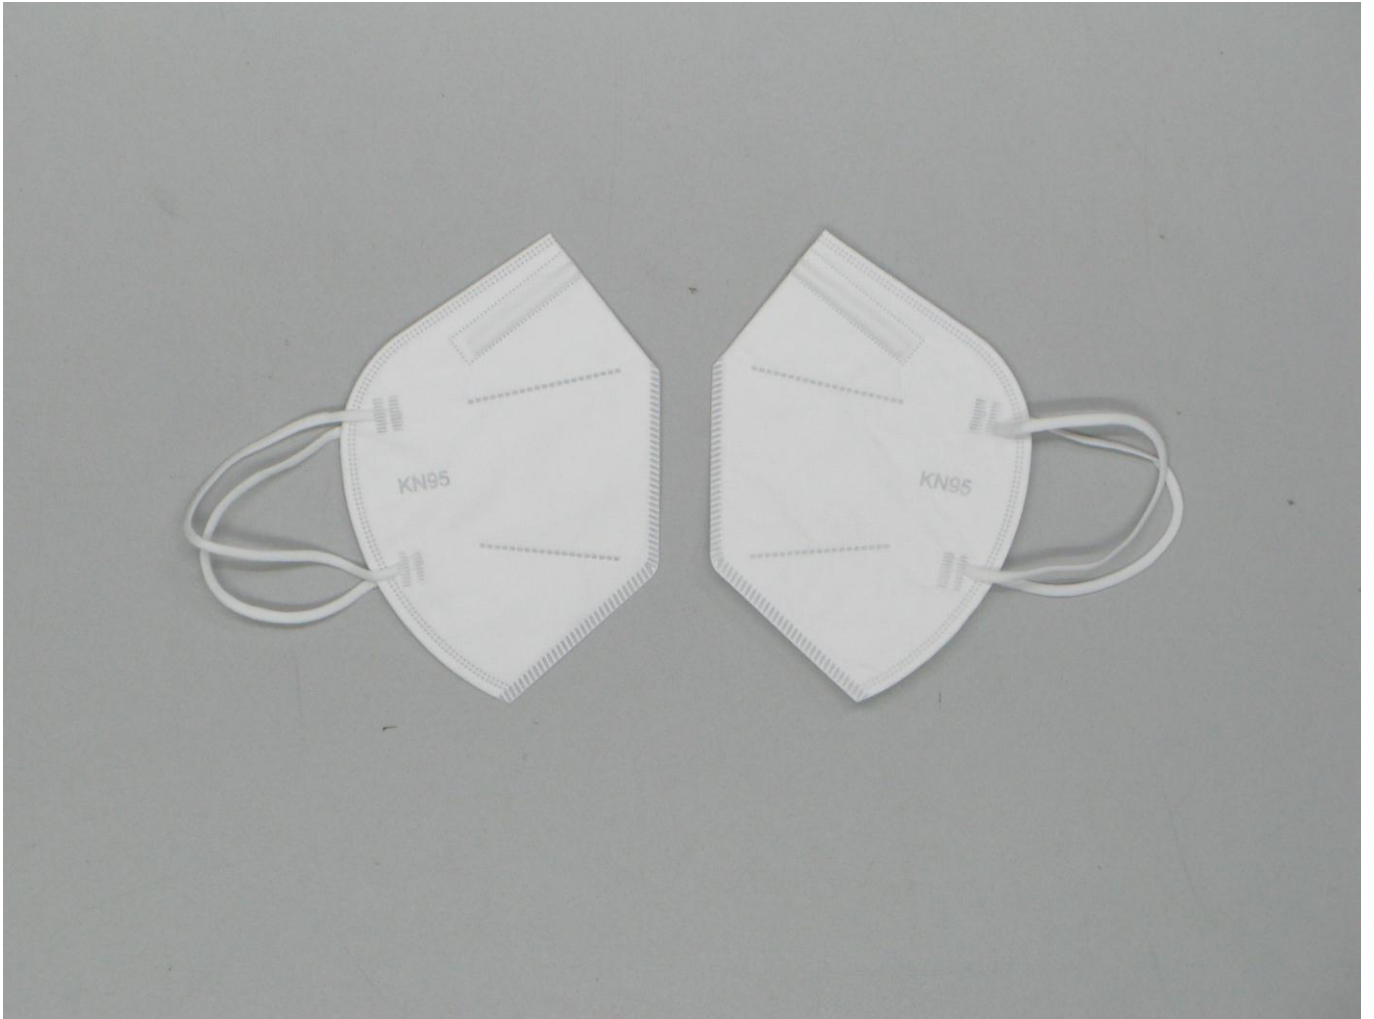

# TEST REPORT

(Electronic version)

No:200081167

## FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m<sup>3</sup>,  
TEMP:23.1℃, RH:36.0%)

### FILTRATION EFFICIENCY(%) :

#### UNTREATED SAMPLE

1# 99.345  
2# 99.470  
3# 99.318  
4# 99.516  
5# 99.482  
6# 99.732  
7# 99.580  
8# 99.521  
9# 99.374  
10# 99.426

#### CONDITIONING TREATED

1# 99.037  
2# 99.145  
3# 99.056  
4# 99.014  
5# 99.214

### REQUIREMENT

#### FILTRATION EFFICIENCY(%) :

≥95.0  
(KN95)  
(GB 2626-2006)

## INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

### UNTREATED SAMPLE:

1# 183.4  
2# 189.2

### PRETREATMENT SAMPLE:

1# 154.9  
2# 150.2

### REQUIREMENT

≤350  
(GB 2626-2006)

## EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

### UNTREATED SAMPLE:

1# 113.3  
2# 117.6

### PRETREATMENT SAMPLE:

1# 103.3  
2# 100.1

### REQUIREMENT

≤250  
(GB 2626-2006)

## APPEARANCE INSPECTION[2 PIECES]

(GB 2626-2006 6.1)

PASS

### REQUIREMENT

ACCORDING TO THE CLAUSE 5.2 OF THE  
PRODUCT STANDARD  
(GB 2626-2006)



—End of Report—

PAGE 4 OF 4